



**>> Passion for
precision <<**

MPS

Multi Platform Systems

OT-SERIES


OSSTEM IMPLANTS

HIOSEN IMPLANT

T-PLUS IMPLANT TECH



MEDENTiKA®
A Straumann Group Brand

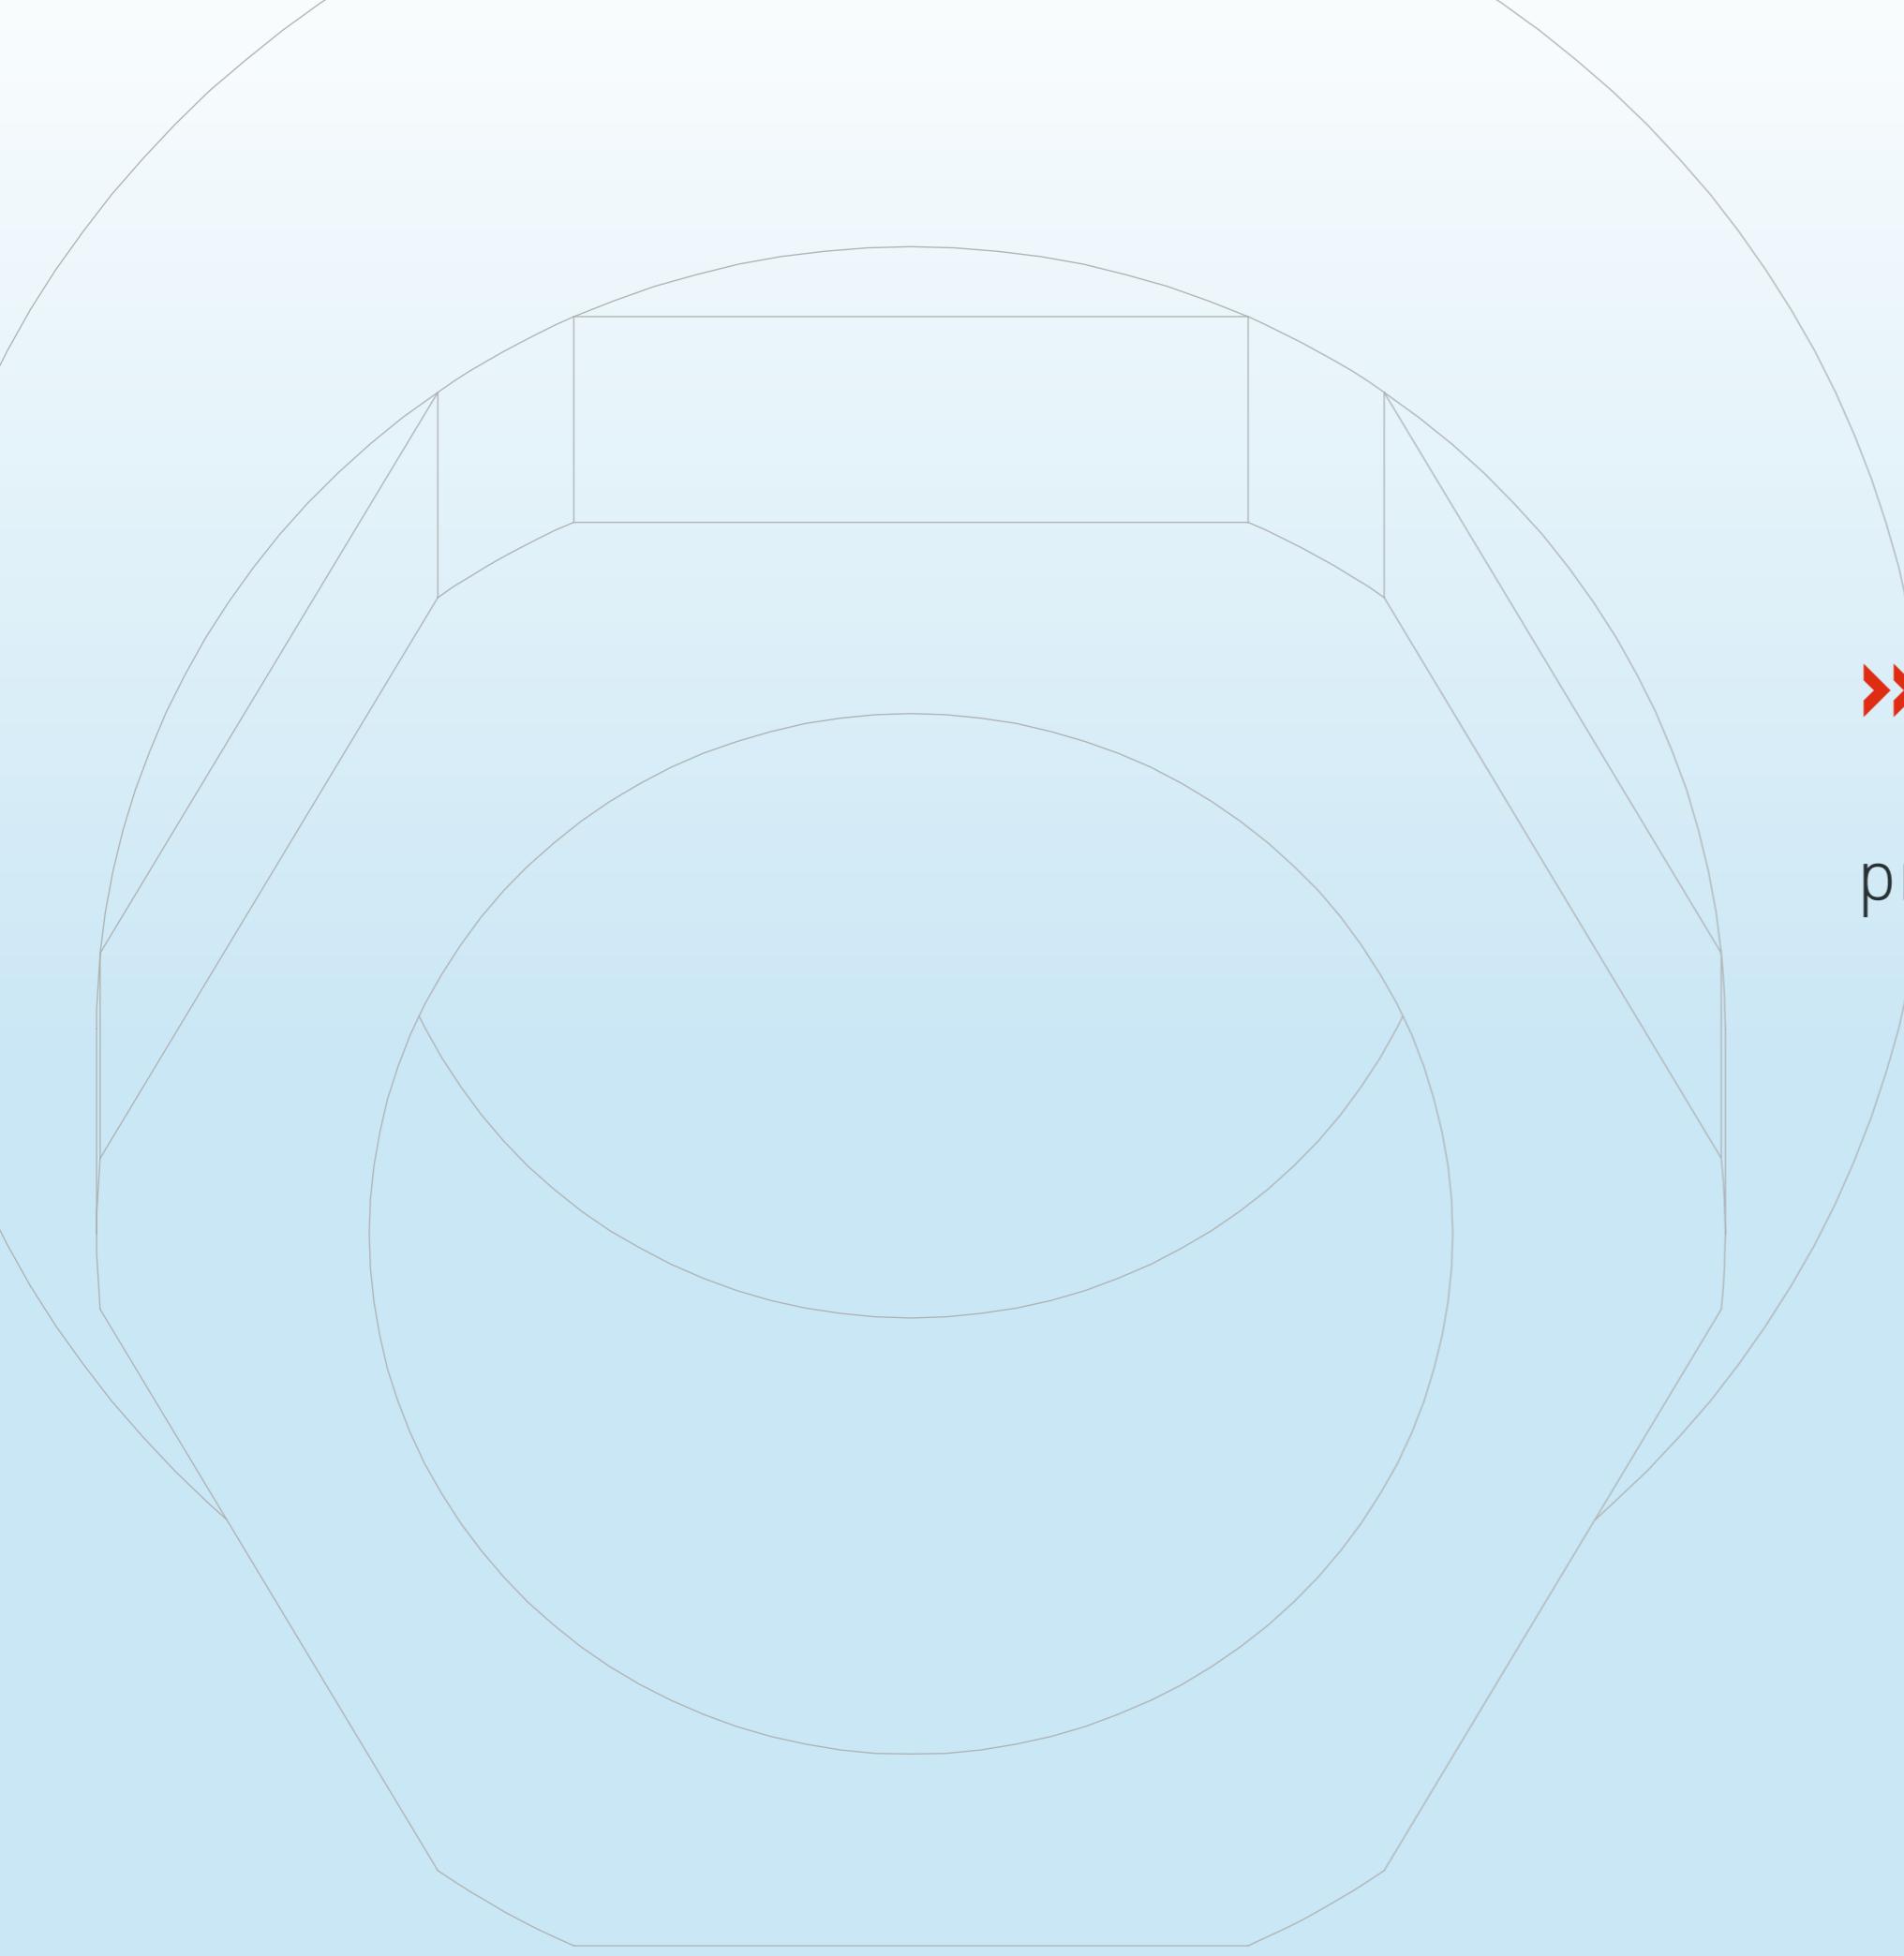

» MEDENTiKA® expands its portfolio of compatible products with the OT Series «

MEDENTiKA® is wholeheartedly committed to continuous development based on the latest findings in challenging implantology.


All products are developed with passion and produced with painstaking attention to detail.

New products are an expression of our comprehensive expertise and take special account of the requirements of our customers and their patients.

>> OT-Series <<

MEDENTiKA® expands its portfolio of compatible products with the OT Series

Compatibility			
OT-Serie	compatibel with	OSSTEM Implants	TS System
		HiOssem Implant®*	ET-System
		T-Plus Implant Tech	A+ Implant
			ST Implant

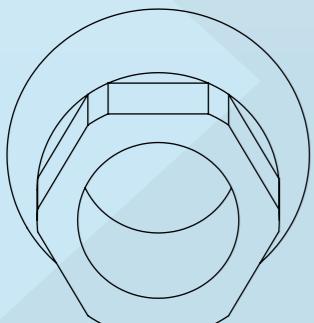

Implant connection:

- M 3.5 mm
- R 4.0-6.0 mm

Portfolio Overview

now available

- Laboratory implant
- Laboratory implant CADCAM
- Placement instrument laboratory implant CADCAM
- Abutment screw
- Laboratory screw
- Scanbody
- Titanium base ASC Flex
- PreFace abutment

coming soon


- Ti-Forms-abutments für M-Series
- Multi-unit abutment
- Novaloc abutment
- Optiloc abutment

>> Scanbody Evolution <<

The latest development from MEDENTiKA®:
The scanbody with a new facelift

SPECIAL SURFACE

Thanks to the special surface,
the use of a scan spray is not
necessary.

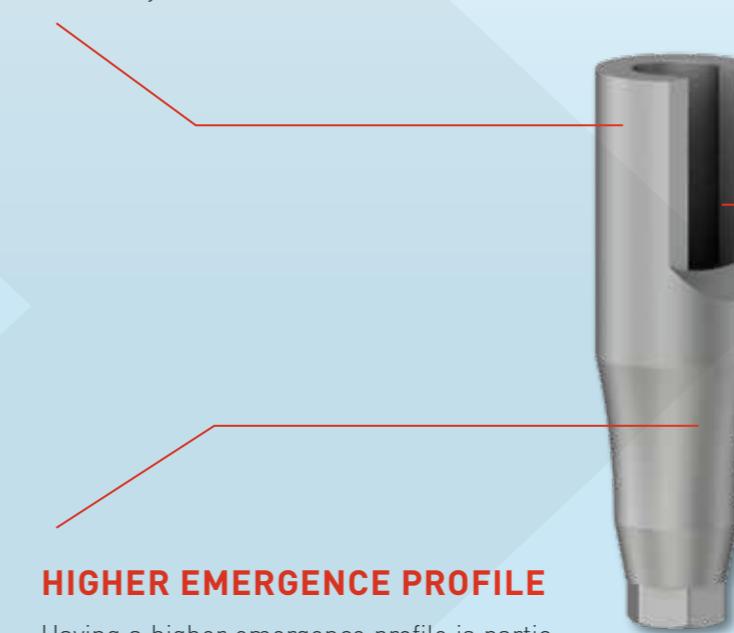


HIGHER EMERGENCE PROFILE

Having a higher emergence profile is particularly necessary for patients with a deeply inserted implant since it ensures that the user has sufficient material for the scan and subsequent adaptation in the CAD software



LATERAL OPENING

Handling is easier for the user,
since the screw is easier to
reach with the screwdriver,
without the need to penetrate
the screw channel from above



Suitable for
chairside and lab side

» MEDENTiKA®
OT-Series «

Product Overview



Laboratory implant


- Titanium Grade 5 CF



Implant connection	M	R
Article No.	OT 50	OT 51

Laboratory implant CADCAM

- Titanium Grade 5 CF



Implant connection	M	R
Article No.	OT 80	OT 81

Please note: This is used for 3D printmodels.

Placement instrument laboratory implant CADCAM

- Stainless steel



Implant connection	M	R
Article No.	OT 80 T	OT 81 T

Abutment screw

- Titanium Grade 5 CF
- Hex 1,2: OT 60 / OT 61
- Ball Torx: OT 62 / OT 63



Article No.	OT 60	OT 61	OT 62	OT 63
-------------	-------	-------	-------	-------

Please note: The correct choice of the abutment screw is stated with the respective abutment in the catalogue.

Laboratory screw

- red coated



Article No.	OT 60 L	OT 61 L
-------------	---------	---------

Please note: The correct choice of the laboratory screw is stated with the respective abutment in the catalogue.

Scanbody

- Titanium
- specially coated
- incl. retention screw




Implant connection

Article No.	OT 1400-L	OT 1410-L
retention screw	OT 60 SB	OT 61 SB

Please note: The Scanbody is sterilisable and for intra-oral scanning.

Titanium base ASC Flex

- angled screw channel
- Titanium Grade 5 CF
- incl. abutment screw
- Type SF = Screw channel angled over the flat of the scanbody Type
- Recommended torque:
20 Ncm: M
30 Ncm: R



Implant connection	M	R
--------------------	---	---

Chimney height 3,5-6,5 mm

Gingiva height 1,0 mm

Article No. Type OT 1600-1-SF OT 1610-1-SF

1/SF

Abutment screw OT 62 OT 63

Please note: To screw in the titanium base ASC Flex you need the Placement instrument Ball-Torx M 03-8 or M 10-8. To select the desired direction of the angled screw channel, please consider the Instruction for use.

PreFace abutment

- Titanium Grade 5 CF
- incl. abutment screw
- Recommended torque:
20 Ncm: M
30 Ncm: R


Implant connection	M	R
--------------------	---	---

Diameter 11,5 mm

Article No. OT 9000-R OT 9010-R

Abutment screw OT 60 OT 61

Laboratory screw OT 60 L OT 61 L



PreFace abutment

- CrCo alloy / CTE 14.1
- incl. abutment screw
- Recommended torque:
20 Ncm: M
30 Ncm: R


Implant connection	M	R
--------------------	---	---

Diameter 11,5 mm

Article No. OT 9800-R OT 9810-R

Abutment screw OT 60 OT 61

Laboratory screw OT 60 L OT 61 L




TI-Forms-Abutment for M-Series

- Titanium Grade 5 CF
- incl. abutment screw
- Recommended torque: 20 Ncm: M
30 Ncm: R

Implant connection	M	R
Diameter	11,5 mm	11,5 mm
Abutment screw	OT 60	OT 61
Laboratory screw	OT 60 L	OT 61 L
Article No.	OT 9000-ST	OT 9010-ST

Please note: This is used with Straumann/M-series.



Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 30 Ncm

Implant connection	M	M	M
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Article No.	OT 8000	OT 8001	OT 8002



Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 30 Ncm

Implant connection	R	R	R
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Article No.	OT 8010	OT 8011	OT 8012



Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 20 Ncm



Implant connection	M	M	M
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	OT 8100	OT 8101	OT 8102



Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 20 Ncm



Implant connection

Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	OT 8300	OT 8301	OT 8302
Abutment screw	OT 62	OT 62	OT 62



Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 30 Ncm



Implant connection

Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	OT 8110	OT 8111	OT 8112
Abutment screw	OT 63	OT 63	OT 63



Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 30 Ncm



Implant connection


Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	OT 8310	OT 8311	OT 8312
Abutment screw	OT 63	OT 63	OT 63



Multi-unit prosthetic components

- OT 8501 Multi-unit bridge screw Hex 1,2
- OT 8508 Multi-unit titanium base incl. bridge screw
- OT 8505 Multi-unit titanium cap incl. bridge screw
- OT 8506 Multi-unit gold cap, castable incl. bridge screw
- OT 8507 Multi-unit CoCr cap incl. bridge screw
- Recommended torque: 15 Ncm

Material	Titanium Grade 5 CF	Titanium Grade 5 CF	Titanium Grade 5 CF	"[AU 60%; Pd 20%; Pt 19%; Ir 1%]"	CrCo alloy / CTE 14.1
Article No.	OT 8501	OT 8508	OT 8505	OT 8506	OT 8507

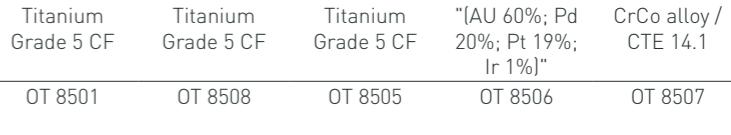

Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw



Version	straight	angled
Article No.	OT 8500	OT 8513

Please note: The Scanbody is sterilisable and for intra-oral scanning.

Multi-unit accessories

- OT 8502 Multi-unit cover cap Hex 1,2
- OT 8503 Multi-unit implant pick-up incl. retention screw



Article No.	OT 8502	OT 8503
-------------	---------	---------

Novaloc abutment straight

- Titanium Grade 5 CF
- ADLC coated
- Recommended torque: 30 Ncm



Implant connection	M	M	M	M	M
Gingiva height	1,0 mm	2,0 mm	3,0 mm	4,0 mm	5,0 mm
Article No.	OT 6000	OT 6100	OT 6200	OT 6300	OT 6400

Please note: To screw in the straight Novaloc abutments you need the original Placement instrument of the respective series.

Novaloc abutment straight

- Titanium Grade 5 CF
- ADLC coated
- Recommended torque: 30 Ncm



Implant connection	R	R	R	R	R
Gingiva height	1,0 mm	2,0 mm	3,0 mm	4,0 mm	5,0 mm
Article No.	OT 6010	OT 6110	OT 6210	OT 6310	OT 6410

Please note: To screw in the straight Novaloc abutments you need the original Placement instrument of the respective series.

Novaloc abutment angled 15°

- Titanium Grade 5 CF
- ADLC coated
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 20 Ncm



Implant connection	M	M	M	M	M
--------------------	---	---	---	---	---

Gingiva height (mm)

Article No.

Abutment screw

Please note: To screw in the angled Novaloc abutments you need the special Placement instrument Ball-Torx M 03-8 or M 10-8.

Novaloc abutment angled 15°

- Titanium Grade 5 CF
- ADLC coated
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 30 Ncm



Implant connection	R	R	R	R	R
--------------------	---	---	---	---	---

Gingiva height (mm)

Article No.

Abutment screw

Please note: To screw in the angled Novaloc abutments you need the special Placement instrument Ball-Torx M 03-8 or M 10-8.

Optiloc abutment straight

- Titanium Grade 5 CF
- ADLC coated
- Recommended torque: 30 Ncm



Implant connection	M	M	M	M	M
--------------------	---	---	---	---	---

Gingiva height

Article No.

Please note: To screw in the straight Optiloc abutments you need the special Placement instrument M 59.

Optiloc abutment straight

- Titanium Grade 5 CF
- ADLC coated
- Recommended torque: 30 Ncm



Implant connection	R	R	R	R	R
--------------------	---	---	---	---	---

Gingiva height

Article No.

Please note: To screw in the straight Optiloc abutments you need the special Placement instrument M 59.

Tools <>

Placement instrument

Hex 1,2

- Hardened stainless steel



Version	Contra-angle	Contra-angle	Manual and ratchet	Manual and ratchet
Type	long	short	long	short
Article No.	M 03-2	M 09-2	M 10-2	M 11-2

Placement instrument

Novaloc abutment, angled

- Hardened stainless steel
- Ball Torx



Version	Contra-angle	Manual and ratchet
Article No.	M 03-8	M 10-8

Placement instrument

Optiloc abutment

- Hardened stainless steel



Version	Contra-angle	Manual and ratchet
Article No.	M 79	M 59

Placement instrument

Multi-unit abutment straight

- Stainless steel



Version	Manual and ratchet
Article No.	M 11-11



NOWOŚĆ

ŁĄCZNIKI MEDENTIBASE

Korzystanie z łącznika MedentiBASE daje możliwość wytwarzania najbardziej skomplikowanych wielopunktowych prac w technologii konwencjonalnej lub CAD/CAM. Można wybierać między bezpośrednio dokręcanymi konstrukcjami mostów i belek lub dokręcaną pośrednią frezowaną belką na łącznikach MedentiBASE oraz na niej biernie dopasowaną suprastukturą.

Łączniki MedentiBASE dostępne są w 5 różnych wysokościach przeształstowych.

KOMPONENTY PROTETYCZNE MEDENTIBASE

MedentiBASE czapeczka tytanowa

MedentiBASE czapeczka plastikowa

MedentiBASE czapeczka złota do odlewów

MedentiBASE podstawa tytanowa

Podstawa tytanowa MedentiBase jest dostępna w wysokości komina 3,5 mm. Nadaje się jako filar do utrzymywania klejonych mostów wielopunktowych, w szczególności wykonanych z materiałów ceramicznych i kompozytów. Do cyfrowych projektów dostępna jest baza Biblioteki Medentika.

MedentiBASE podstawa klejona

Podstawy MedentiBASE są dostępne w wysokości 3,0 mm (krótką) i 4,00 mm (długa). Mogą być używane do tworzenia wielopunktowych przykręcanych mostów i belek z metalu, gdzie istotna jest pasywność konstrukcji. Do cyfrowych projektów dostępna jest baza Biblioteki Medentika.

MedentiBASE scanbody

MedentiBASE scanbody mogą być stosowane do skanowania modelu celem wykonania jego cyfryzacji. Biblioteka MedentiBASE, która jest niezbędna do projektowania jest oczywiście bezpłatna. Obecnie jest dostępna dla 3Shape, Dentalwings i Exocad.

KOMPONENTY MEDENTIBASE

Z lewej do prawej:

MedentiBASE śruba gojąca

MedentiBASE transfer wyciskowy

MedentiBASE analog laboratoryjny

MedentiBASE przenośnik M11-4



» **Każdy, kto pracuje z komponentami Medentika jest w bezpiecznych rękach.** Gwarancja obejmuje nie tylko jakość i trwałość łączników, ale również implanty innych producentów. «

MEDENTIKA nie tylko zapewnia 10-letnią gwarancję dla wszystkich łączników Medentika i MedentiCAD z tytanu (w tym śruby mocujące) produkowanych i dostarczanych przez MEDENTIKA, **ale również gwarancję na implanty innych producentów używane z łącznikiem.** Przypadki z natychmiastowymi obciążeniami są wyłączone z niniejszej gwarancji.

Gwarancja dla implantów obowiązuje na przykład w sytuacji, gdy producent implantu ogranicza swoje warunki gwarancji na wszczep, ponieważ łączy się on z łącznikiem MEDENTIKA lub MedentiCAD. Aby uzyskać więcej informacji prosimy o zapoznanie się z warunkami gwarancji, które chętnie wyjaśnimy.

Możesz na nas liczyć.





Publisher: MEDENTiKA® GmbH
Hammweg 8-10
76549 Hugelsheim
Tel: +49 (0)7229 69912-10
info@medentika.de
www.medentika.com

Design: Der WeberFink GbR
graphic design studio
www.weberfink.de

Date: June 2019

We are certified:
DIN EN ISO 13485
Medical Device Directive 93/42/EEC
Annex II

CE0483

Technical changes and errors reserved.

You can find the Instructions for use and warranty conditions on the website www.medentika.com

More information on the warranty can also be requested directly from the manufacturer

