

MPS

MULTI PLATFORM SYSTEMS

Multi-unit abutments



Multi-unit abutment

The multi-unit abutment supports a wide range of prosthetic restorations. So it's ideal for producing personalized multi-unit restorations, for example, or as a basis for customized restorations with implant-borne fixed full dentures according to the full arch treatment concept.



The multi-unit product range is regularly expanded with additional implant connections.

Available for a wide range of implant systems:

Manufacturer	Implant system	compatible with
BioHorizons	Tapered Internal	R-Series
	Tapered Internal Plus	R-Series
	Tapered Tissue Level	R-Series
BIOMET 3i	Certain***	H-Series
Camlog	Camlog**	C-Series
Dentium	SuperLine	DT-Series
	Implantium	DT-Series
	Implantium II	DT-Series
DENTSPLY SIRONA	ANKYLOS** C/X	Y-Series
	ASTRA TECH OsseoSpeed EV	EV-Series
HiOssen Implant**	ET System	OT-Series
MIS	SEVEN Internal Hex	R-Series
Nobel Biocare	NobelActive**	F-Series
	NobelReplace** Conical	F-Series
OSSTEM Implants	TS System	OT-Series
Straumann	Bone Level	L-Series
	Tissue Level	N-Series
T-Plus Implant Tech	A+ Implant	OT-Series
	ST Implant	OT-Series
Zimmer Dental	Tapered Screw-Vent**	R-Series

All multi-unit abutments, incl. insertion aid, are delivered sterile-packed.

A wide range of options exists for prosthetic restorations.

- Bonding of titanium bases in full dentures as a temporary solution.
- Production of superstructure frameworks with CoCr or HSL caps.
- CAD/CAM milled bars or bridges.
- Full arch treatment concept

Full denture

A provisional full denture is prepared appropriately in the area of the titanium bases and then placed on the model and/or inserted in the mouth free of tension.



Final bridge restoration on two implants in the posterior region

A metal framework is prepared appropriately in the area of the titanium bases and then bonded in the mouth free of tension. Alternatively, directly cast HSL or CoCr bases can be used to prepare the framework. After final preparation, the bridge is screw-retained occlusally.

This procedure is also suitable for preparing a final full restoration on at least four implants in the mandible or six implants in the maxilla.



Bar with removable full denture


An individually milled or CAD/CAM fabricated bar is screwed onto the multi-unit abutments. The final removable restoration can now be completed according to the respective indication and the patient's wishes.



The full arch treatment concept

The full arch treatment concept is a special treatment concept for an implant-borne, fixed, full-arch restoration for edentulous patients with an atrophic alveolar ridge on two straight and two 30 degree-angled implants.

The temporary restoration is immediately screwed onto the implants with the multi-unit abutments. The straight and 30 degree-angled multi-unit abutments allow a common insertion path for the prosthetic restoration.

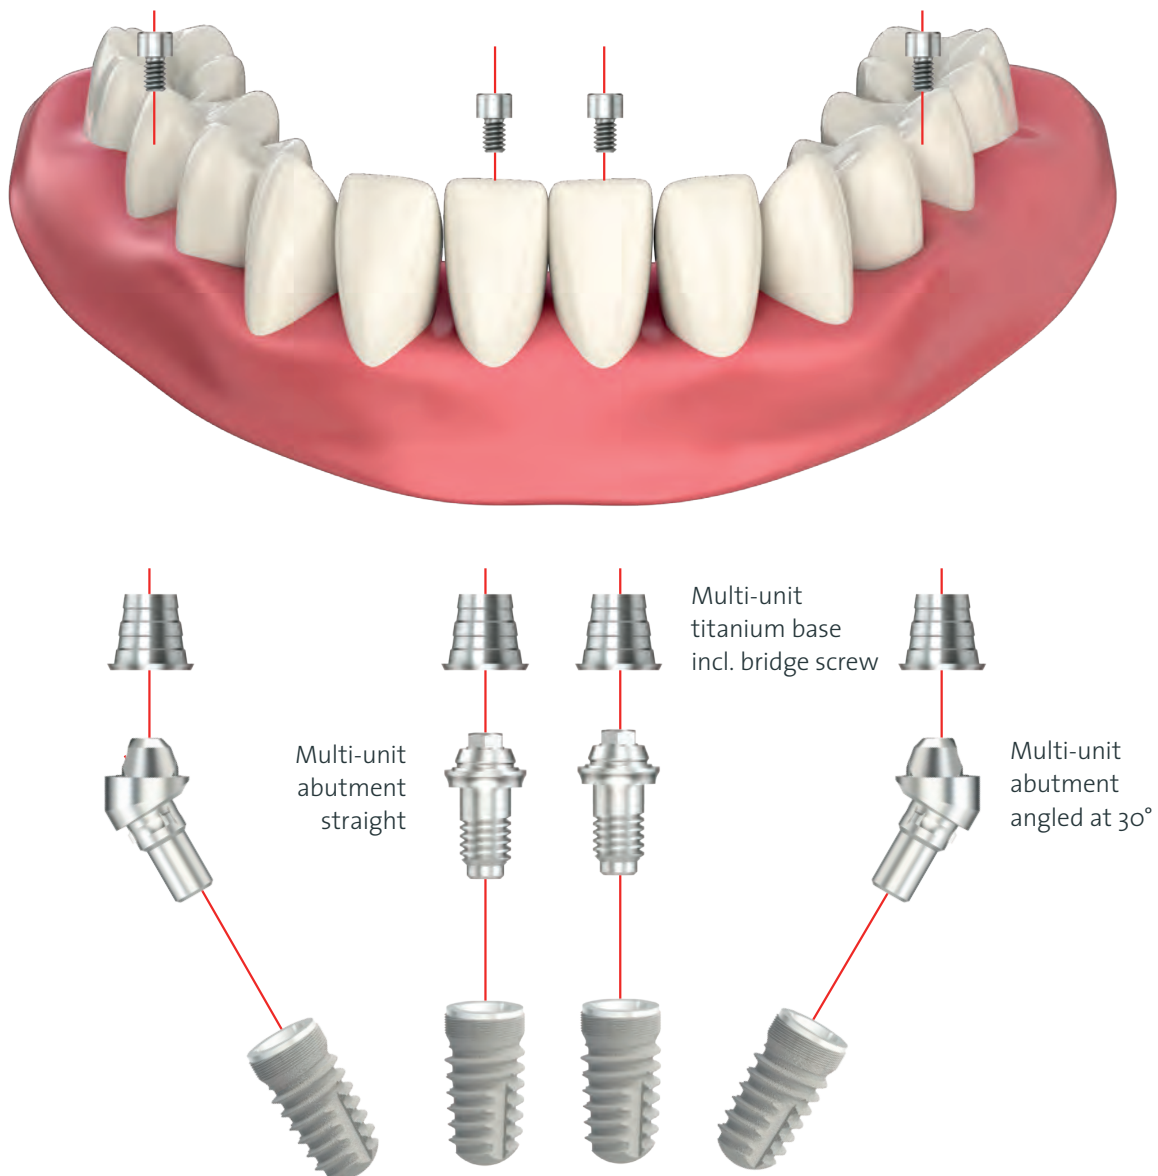

Multi-unit abutments



Treatment options

Various prosthetic components are available for the different treatment options.

Gingival height

The multi-unit abutments are available in different gingival heights.

Implant connection


Available with the implant connections of the major implant manufacturers.

Multi-unit divergence compensation

The multi-unit abutments share a uniform platform for prosthetic components with a taper of 21° (on one side).

If the 30 degree-angled multi-unit abutments are used, compensation of divergences between implants of up to 102° is possible.

This results from the respective 30 degree angulation of the multi-unit abutments and the platform taper of 21° .

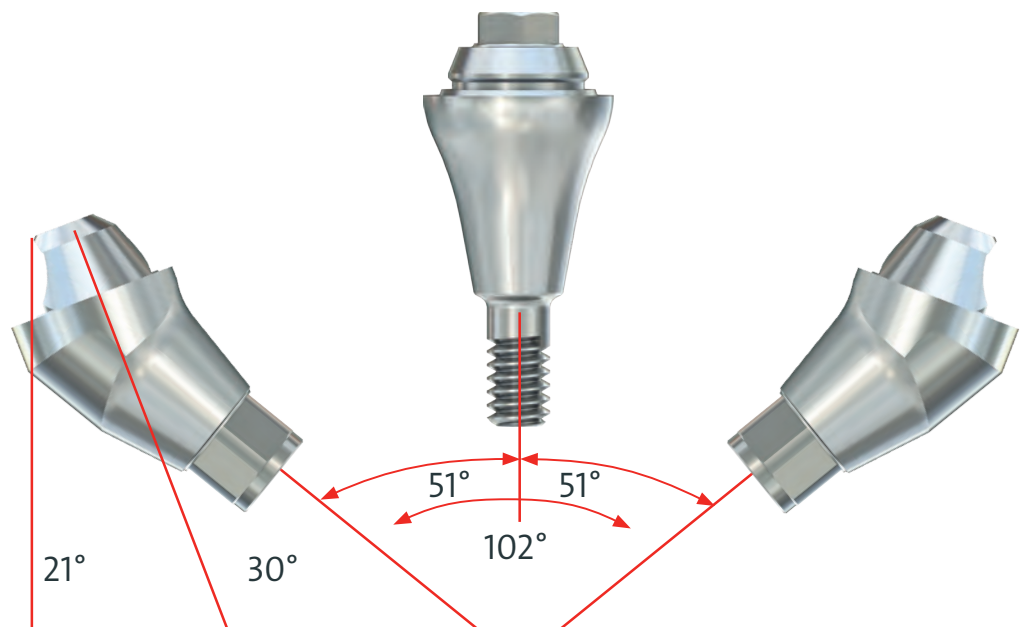

NEW

Now with optimized, soft-tissue-sparing emergence profile depending on the implant interface.

Treatment options

Various prosthetic components are available for the different treatment options.

Gingival height

The multi-unit abutments are available in different gingival heights.

Implant connection

Available with the implant connections of the major implant manufacturers.

Two angulations

The multi-unit abutments are available with angulations of 17° and 30°.



Angulation	Variant		Gingival height (GH)*
Straight			low
			medium
			high
17°	Type 1: over flat 	Type 2: over corner 	low
			medium
			high
30°	Type 1: over flat 	Type 2: over corner 	low
			medium
			high

*Exact lengths depend on the implant system, see list on the following pages

Multi-unit prosthetic components

digital

conventional



Bridge screw

for any cap and including the titanium base



Titanium base

for insertion in the bridge/prosthesis (passive fit) incl. bridge screw



Titanium cap

for individual cutting to length and insertion in the bridge or prosthesis, or for the fabrication of temporary restorations, incl. bridge screw

conventional



Modeling sleeve

for modeling on the titanium cap or titanium base, only for use in combination with the titanium base or titanium cap



gold cap, castable

for casting gold alloys, incl. bridge screw



CoCr cap

for casting non-precious alloys, incl. bridge screw

Digital libraries are available for the following manufacturers*:

3shape

exocad

dental wings
A Straumann Group Brand

NEW



Titanium base ASC

for insertion in the bridge/prosthesis with angled screw channel



Titanium cap Flex

for cutting to length for optimal use in the digital workflow.



Multi-unit screw patrix MedentiLOC and Novaloc

the new multi-unit screw patrix gives you yet another option for restoration.

* to some extent this depends on the availability of the updates of the specific manufacturer.


Multi-unit prosthetic components

Multi-unit screw matrix MedentiLOC/Novaloc

The new multi-unit screw matrix offers you yet another option for restoration. It enables you to switch easily from a screw-retained restoration to a removable overdenture construction.

Screw slot

The integrated screw in the screw matrix matches the screwdriver for the respective implant system.

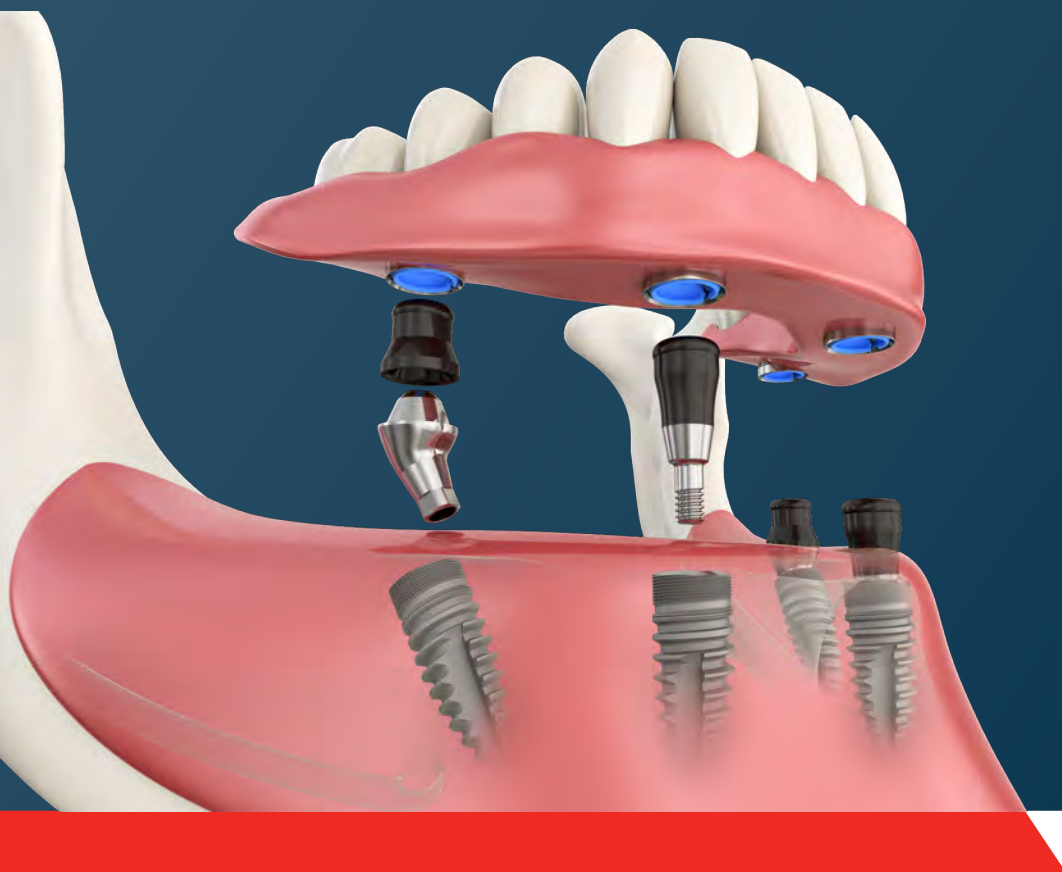

Digital libraries are available for the following manufacturers*:

3shape

exocad

dental wings
A Straumann Group Brand

Placement instrument

The supplied bridge screw incorporates the proven slot for the Ball-Torx placement instrument M 03-8 , M 10-8 or 6-13-06.



Titanium cap Flex

The titanium cap Flex offers a variable chimney height. The 14.5 mm chimney height also supports high restorations, whether for a provisional or definitive restoration. However, this can be individually shortened in 2 mm increments to 4.5 mm. The different chimney heights are defined in the CAD library.



Titanium base ASC

For unfavorably positioned implants or in an esthetically demanding site, the screw channel can optionally be moved to the non-visible area.

* to some extent this depends on the availability of the updates of the specific manufacturer.

Laboratory implants multi-unit abutments



Laboratory implant

for use in conventional model fabrication



Laboratory implant angled

for use in conventional model fabrication

Angled at 17° + 30°.



Laboratory implant CAD/CAM

for use in digital model fabrication (printed model)



Laboratory implant CAD/CAM angled


for use in digital model fabrication (printed model) Angled at 17° + 30°

Multi-unit accessories



Scanbody

Straight multi-unit for taking digital impressions of straight multi-unit abutments

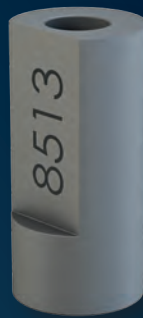


Scanbody

Angled multi-unit for taking digital impressions of the angled multi-unit abutments 17° and 30°



Implant pick-up

for taking impressions of multi-unit abutments



Cover cap

for protecting the abutments during the healing phase

Placement instrument


for the straight multi-unit abutments



How it's done

Straight multi-unit abutment


After the implant is inserted, the straight multi-unit abutment is connected to the implant using the special insertion aid that is already fixed on the abutment, and the abutment is then tightened with the placement instrument to the torque setting for the corresponding system.

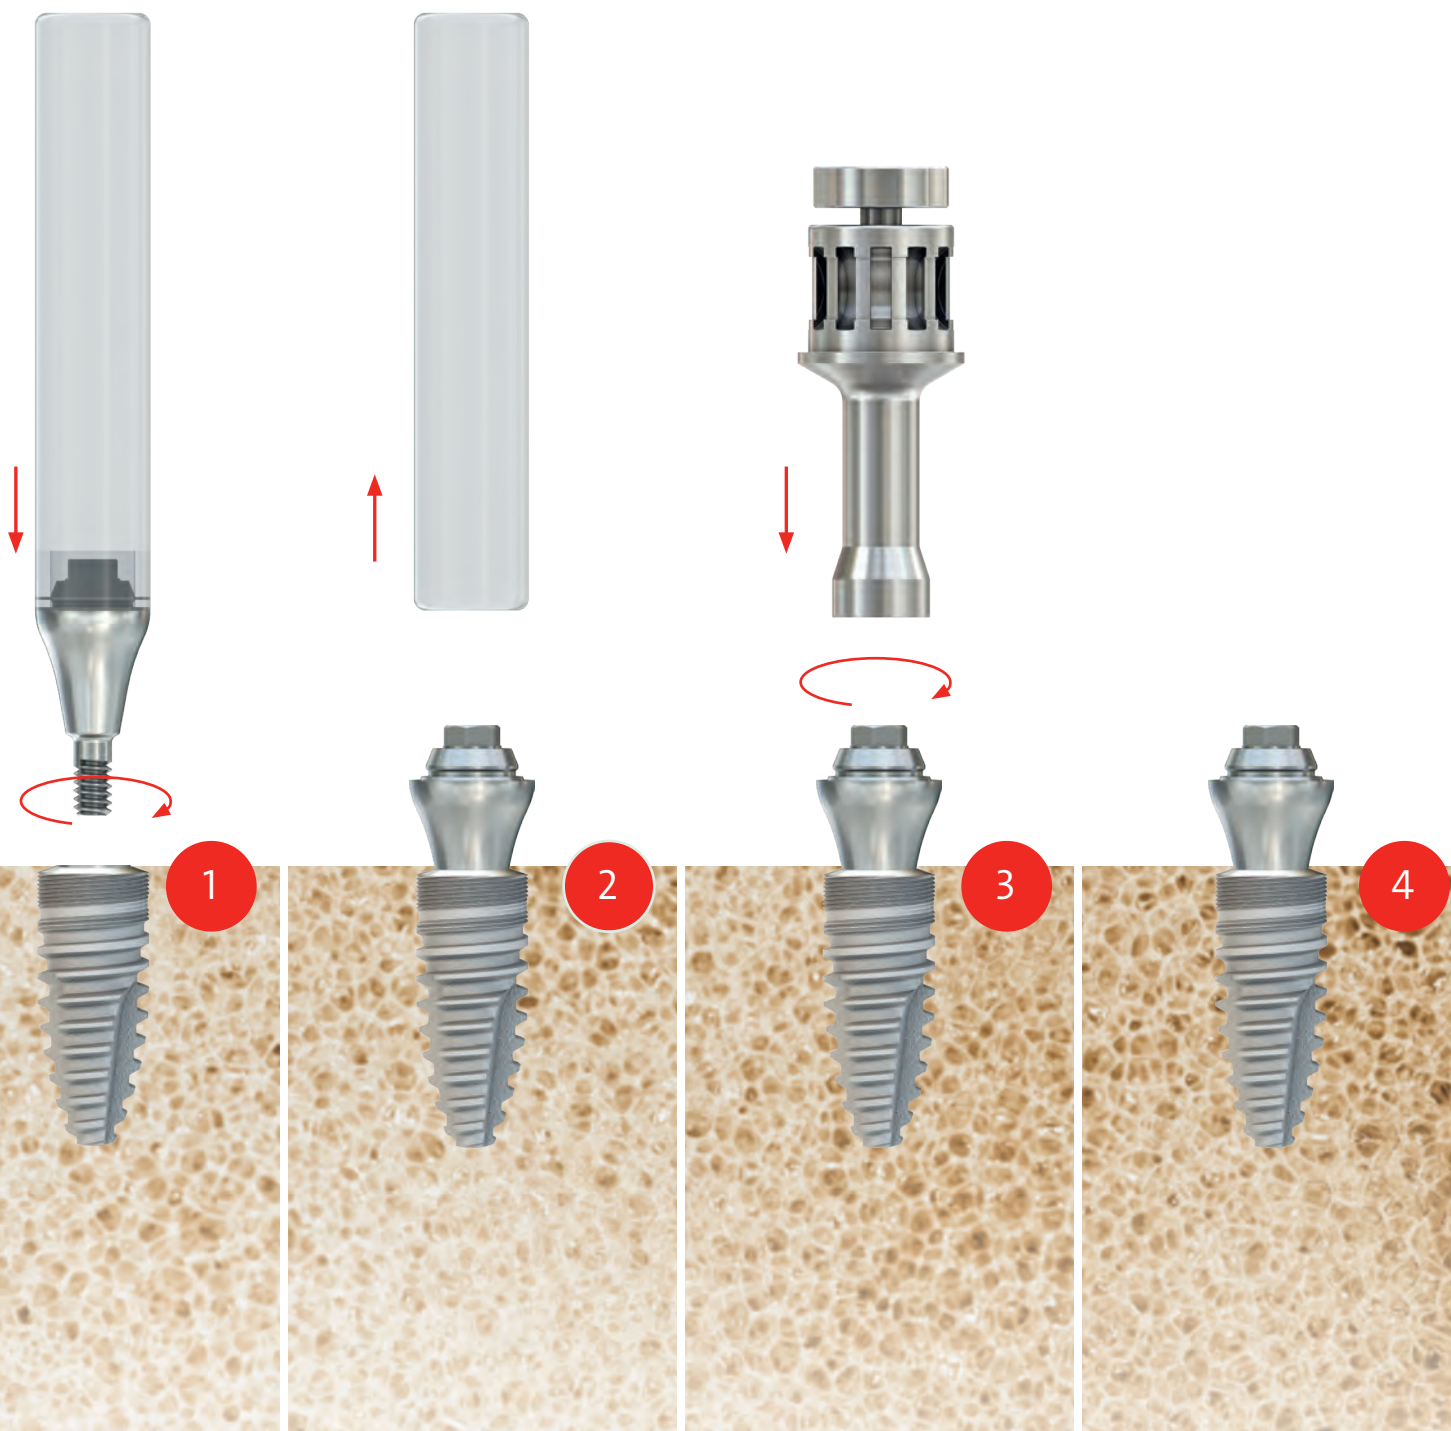

How it's done

Angled multi-unit abutment

After the implant is inserted, the angled multi-unit abutment is connected to the implant using the special insertion aid that is already fixed on the abutment, and the abutment screw is then tightened to the torque setting for the corresponding system.

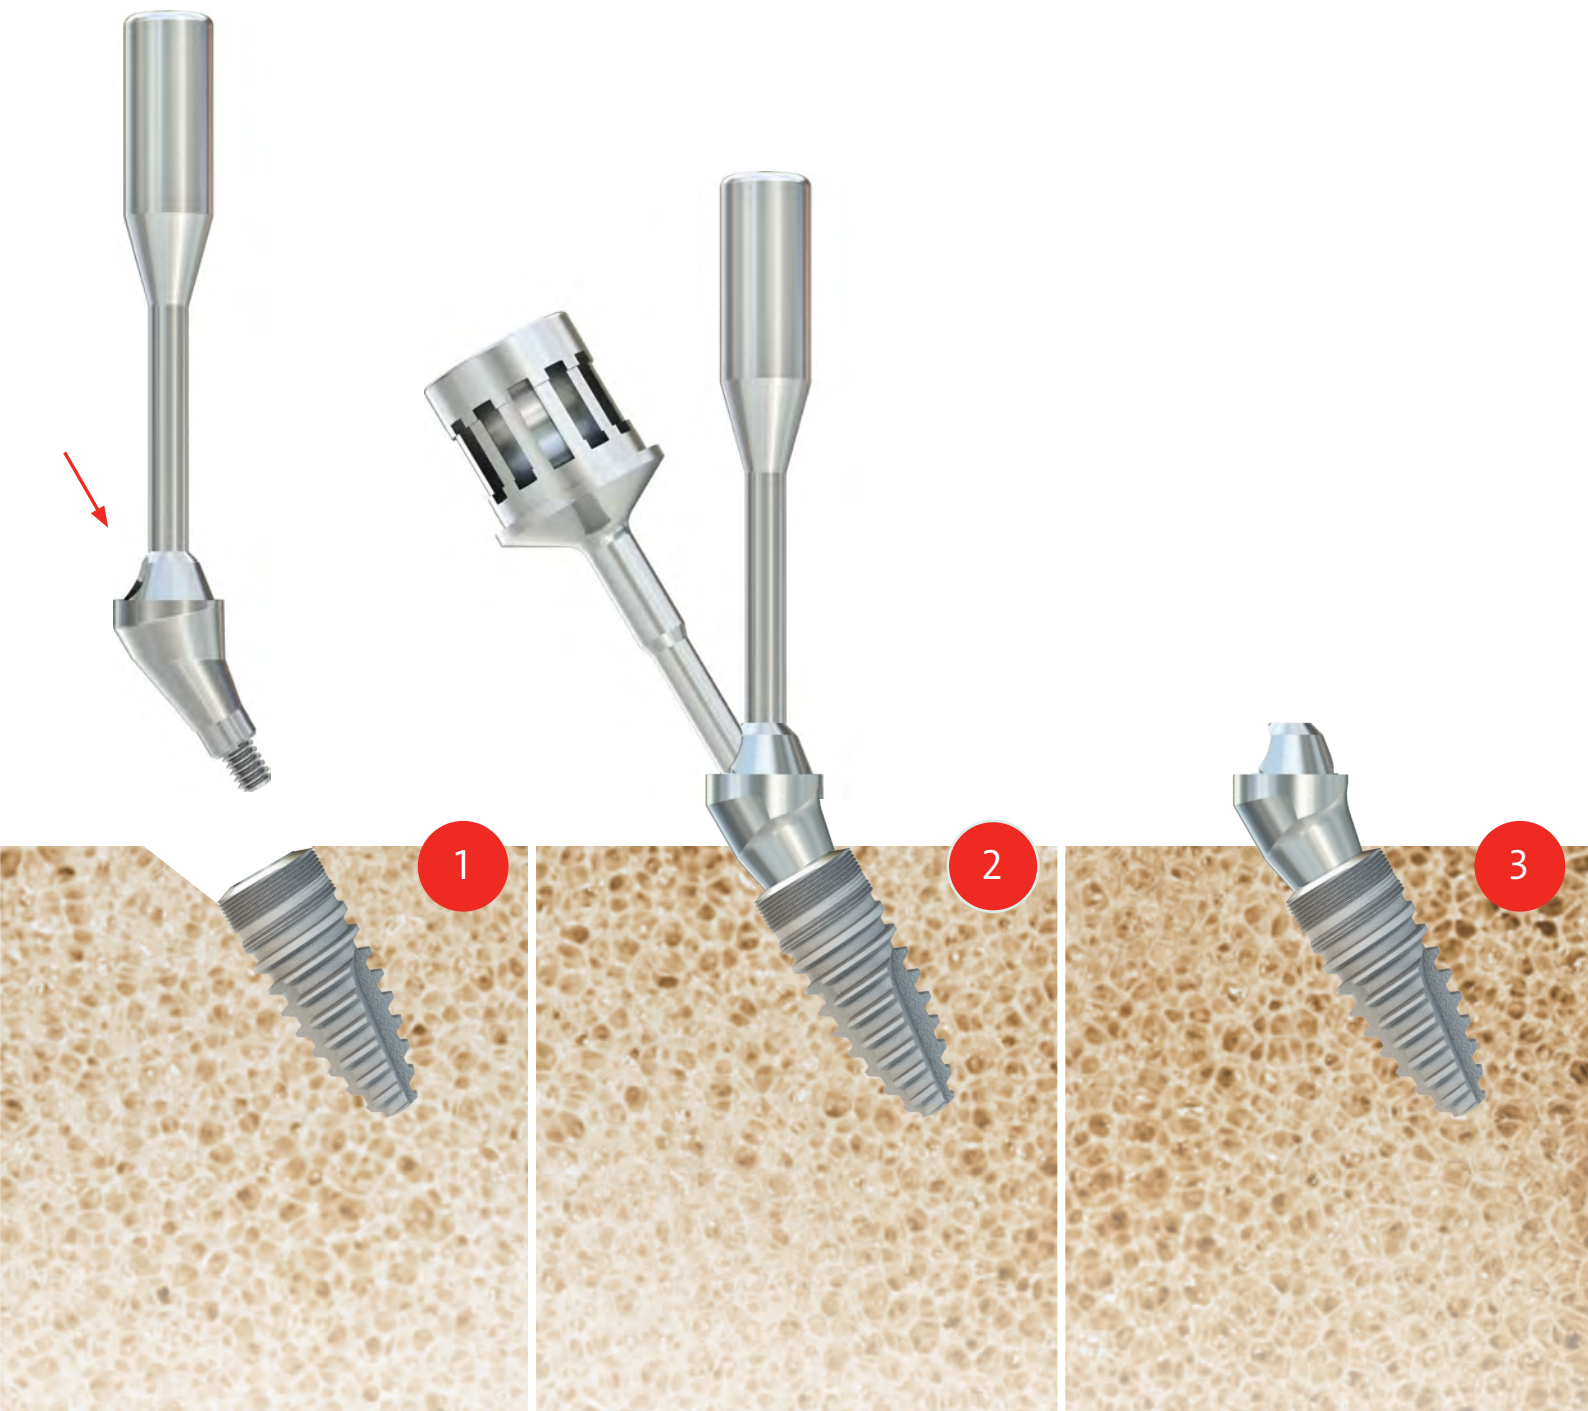


All multi-unit abutments, including the insertion aid, are delivered sterile-packed.



Medentika® Multi-unit abutments

Product overview

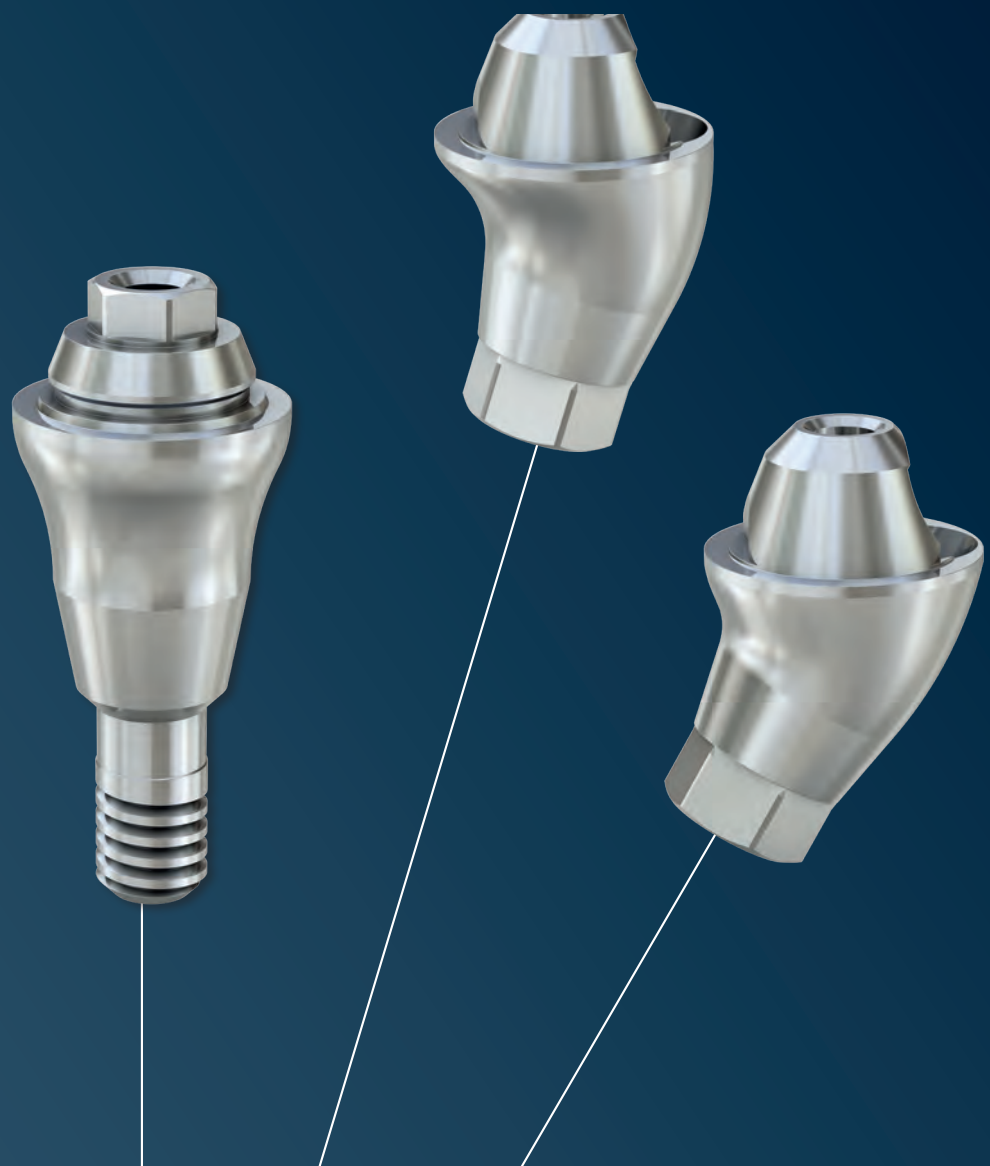

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 20 Ncm



Implant connection	D 3,3	D 3,3	D 3,3
Gingiva height	1,0 mm	3,0 mm	5,0 mm
Article No.	C 8000	C 8001	C 8002

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 30 Ncm



Implant connection	D 3,8	D 3,8	D 3,8
Gingiva height	1,0 mm	3,0 mm	5,0 mm
Article No.	C 8010	C 8011	C 8012

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 30 Ncm



Implant connection	D 4,3	D 4,3	D 4,3
Gingiva height	1,0 mm	3,0 mm	5,0 mm
Article No.	C 8020	C 8021	C 8022

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 30 Ncm




Implant connection	D 5,0	D 5,0	D 5,0
Gingiva height	1,0 mm	3,0 mm	5,0 mm
Article No.	C 8030	C 8031	C 8032

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over cam
- Recommended torque: 20 Ncm



Implant connection	D 3,3	D 3,3	D 3,3
Gingiva height (mm)	1,1/2,5	2,1/3,5	3,6/5,0
Article No. Type 1	C 8100	C 8101	C 8102
Article No. Type 2	C 8200	C 8201	C 8202
Abutment screw	C 64	C 64	C 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over cam
- Recommended torque: 20 Ncm



Implant connection	D 3,3	D 3,3	D 3,3
Gingiva height (mm)	0,6/3,0	1,6/4,0	2,4/5,0
Article No. Type 1	C 8300	C 8301	C 8302
Article No. Type 2	C 8400	C 8401	C 8402
Abutment screw	C 64	C 64	C 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over cam
- Recommended torque: 20 Ncm




Implant connection	D 3,8	D 3,8	D 3,8
Gingiva height (mm)	1,1/2,5	2,1/3,5	3,6/5,0
Article No. Type 1	C 8110	C 8111	C 8112
Article No. Type 2	C 8210	C 8211	C 8212
Abutment screw	C 64	C 64	C 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over cam
- Recommended torque: 20 Ncm



Implant connection	D 3,8	D 3,8	D 3,8
Gingiva height (mm)	0,6/3,0	1,6/4,0	2,4/5,0
Article No. Type 1	C 8310	C 8311	C 8312
Article No. Type 2	C 8410	C 8411	C 8412
Abutment screw	C 64	C 64	C 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over cam
- Recommended torque: 20 Ncm



Implant connection	D 4,3	D 4,3	D 4,3
Gingiva height (mm)	1,1/2,5	2,1/3,5	3,6/5,0
Article No. Type 1	C 8120	C 8121	C 8122
Article No. Type 2	C 8220	C 8221	C 8222
Abutment screw	C 64	C 64	C 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over cam
- Recommended torque: 20 Ncm



Implant connection	D 4,3	D 4,3	D 4,3
Gingiva height (mm)	0,6/3,0	1,6/4,0	2,4/5,0
Article No. Type 1	C 8320	C 8321	C 8322
Article No. Type 2	C 8420	C 8421	C 8422
Abutment screw	C 64	C 64	C 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over cam
- Recommended torque: 20 Ncm



Implant connection	D 5,0	D 5,0	D 5,0
Gingiva height (mm)	1,1/2,5	2,1/3,5	3,6/5,0
Article No. Type 1	C 8130	C 8131	C 8132
Article No. Type 2	C 8230	C 8231	C 8232
Abutment screw	C 65	C 65	C 65

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over cam
- Recommended torque: 20 Ncm



Implant connection	D 5,0	D 5,0	D 5,0
Gingiva height (mm)	0,6/3,0	1,6/4,0	2,4/5,0
Article No. Type 1	C 8330	C 8331	C 8332
Article No. Type 2	C 8430	C 8431	C 8432
Abutment screw	C 65	C 65	C 65

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Abutment screw

- Titanium Grade 5 CF



Placement instrument	Hex 1,26	Hex 1,26
Article No.	C 64	C 65

Please note: The correct choice of the abutment screw is stated with the respective abutment in the catalogue.

Multi-unit bridge screw






- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Placement instrument	Ball Torx	Hex 1,26
Article No.	6-31-01	C 8501

Multi-unit prosthetic components

- Recommended torque: 15 Ncm
- Titanium base / titanium cap: incl. bridge screw
Material: Titanium Grade 5 CF
- Modelling sleeve without bridge screw
Material: Tecanat (PC)

					
	titanium base ASC	titanium base	titanium cap	titanium cap Flex	modelling sleeve
Article No.	6-31-02	C 8508	C 8505	C 8519	8510
Please note:	The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.				



Multi-unit prosthetic components

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material gold cap, castable: "(AU 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1

		
	gold cap, castable	CoCr cap
Article No.	C 8506	C 8507



Multi-unit screw patrix

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm

		
	MedentiLOC	Novaloc
Article No.	C 8517	C 8518
Please note:	To screw in the screw patrix you need the placement instrument of the respective series.	




Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw

		
	straight	angled
Version	straight	angled
Article No.	C 8500	C 8513
Please note:	The Scanbody is sterilisable and for intra-oral scanning.	

Multi-unit Laboratory implant

- Titanium Grade 5 CF

			
	straight	angled 17°	angled 30°
Version	straight	angled 17°	angled 30°
Type			
Article No.	8504	8514-17	8514-30

Multi-unit Laboratory implant CAD/CAM


- Titanium Grade 5 CF

Version				
Type		straight	angled 17°	angled 30°
Article No.		8509	8515-17	8515-30

Multi-unit accessories

- C 8502 Multi-unit cover cap Hex 1,26
- C 8503 Multi-unit implant pick-up incl. retention screw
- M 11-11 Placement instrument Multi-unit abutment Manual and ratchet
- 8515 T Placement instrument laboratory implant CAD/CAM Multi-unit

Article No.

			
C 8502	C 8503	M 11-11	8515 T

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 25 Ncm



Implant connection	D 3,6-7,0	D 3,6-7,0	D 3,6-7,0
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Article No.	DT 8000	DT 8001	DT 8002

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 25 Ncm

Type 1



Implant connection	D 3,6-7,0	D 3,6-7,0	D 3,6-7,0
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	DT 8100	DT 8101	DT 8102
Abutment screw	DT 63	DT 63	DT 63

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 25 Ncm

Type 1



Implant connection	D 3,6-7,0	D 3,6-7,0	D 3,6-7,0
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	DT 8300	DT 8301	DT 8302
Abutment screw	DT 63	DT 63	DT 63

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Abutment screw

- Titanium Grade 5 CF



Placement instrument	Hex 1,26
Article No.	DT 63

Please note: The correct choice of the abutment screw is stated with the respective abutment in the catalogue.






Multi-unit bridge screw

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm

		
Placement instrument	Ball Torx	Hex 1,26
Article No.	6-31-01	DT 8501



Multi-unit prosthetic components

- Recommended torque: 15 Ncm
- Titanium base / titanium cap: incl. bridge screw
- Material: Titanium Grade 5 CF
- Modelling sleeve without bridge screw
- Material: Tecanat (PC)

					
	titanium base ASC	titanium base	titanium cap	titanium cap Flex	modelling sleeve
Article No.	6-31-02	DT 8508	DT 8505	DT 8519	8510
Please note:	The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.				



Multi-unit prosthetic components

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material gold cap, castable: "(AU 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1

		
	gold cap, castable	CoCr cap
Article No.	DT 8506	DT 8507



Multi-unit screw patrix

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm

		
	MedentiLOC	Novaloc
Article No.	DT 8517	DT 8518
Please note:	To screw in the screw patrix you need the placement instrument of the respective series.	




Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw

		
Version	straight	angled
Article No.	DT 8500	DT 8513
Please note:	The Scanbody is sterilisable and for intra-oral scanning.	

Multi-unit Laboratory implant

- Titanium Grade 5 CF

			
Version	straight	angled	angled
Type		17°	30°
Article No.	8504	8514-17	8514-30


Multi-unit Laboratory implant CAD/CAM

- Titanium Grade 5 CF

			
Version	straight	angled	angled
Type		17°	30°
Article No.	8509	8515-17	8515-30

Multi-unit accessories

- DT 8502 Multi-unit cover cap Hex 1,26
- DT 8503 Multi-unit implant pick-up incl. retention screw
- M 11-11 Placement instrument Multi-unit abutment Manual and ratchet
- 8515 T Placement instrument laboratory implant CAD/CAM Multi-unit

				
Article No.	DT 8502	DT 8503	M 11-11	8515 T

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 25 Ncm



Implant connection	D 3,6	D 3,6	D 3,6
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Article No.	EV 8010	EV 8011	EV 8012

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 25 Ncm



Implant connection	D 4,2	D 4,2	D 4,2
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Article No.	EV 8020	EV 8021	EV 8022

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 25 Ncm



Implant connection	D 4,8	D 4,8	D 4,8
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Article No.	EV 8030	EV 8031	EV 8032

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 25 Ncm

Type 1



Implant connection	D 3,6	D 3,6	D 3,6
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	EV 8110	EV 8111	EV 8112
Abutment screw	EV 64	EV 64	EV 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 25 Ncm

Type 1



Implant connection	D 3,6	D 3,6	D 3,6
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	EV 8310	EV 8311	EV 8312
Abutment screw	EV 64	EV 64	EV 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.



Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 25 Ncm

Type 1



Implant connection	D 4,2	D 4,2	D 4,2
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	EV 8120	EV 8121	EV 8122
Abutment screw	EV 65	EV 65	EV 65

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.



Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 25 Ncm

Type 1



Implant connection	D 4,2	D 4,2	D 4,2
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	EV 8320	EV 8321	EV 8322
Abutment screw	EV 65	EV 65	EV 65

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.



Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 25 Ncm

Type 1



Implant connection	D 4,8	D 4,8	D 4,8
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	EV 8130	EV 8131	EV 8132
Abutment screw	EV 66	EV 66	EV 66

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.



Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 25 Ncm

Type 1



Implant connection	D 4,8	D 4,8	D 4,8
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	EV 8330	EV 8331	EV 8332
Abutment screw	EV 66	EV 66	EV 66

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Abutment screw

- Titanium Grade 5 CF



Placement instrument	Hex 1,26	Hex 1,26	Hex 1,26
Article No.	EV 64	EV 65	EV 66

Please note: The correct choice of the abutment screw is stated with the respective abutment in the catalogue.

Multi-unit bridge screw


- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Placement instrument	Ball Torx	Hex 1,26
Article No.	6-31-01	EV 8501

Multi-unit prosthetic components

- Recommended torque: 15 Ncm
- Titanium base / titanium cap: incl. bridge screw
- Material: Titanium Grade 5 CF
- Modelling sleeve without bridge screw
- Material: Tecanat (PC)

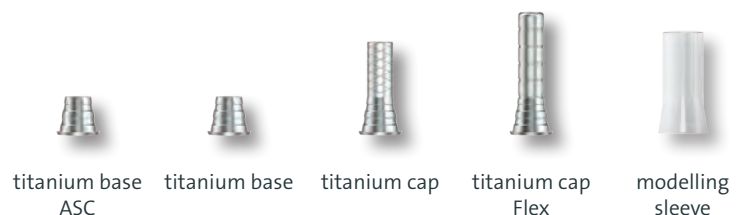

Article No.	6-31-02	EV 8508	EV 8505	EV 8519	8510
-------------	---------	---------	---------	---------	------

Please note: The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.

Multi-unit prosthetic components

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material gold cap, castable: "(AU 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1



Article No.	EV 8506	EV 8507
-------------	---------	---------

Multi-unit screw patrix

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



MedentiLOC

Novaloc

Article No.	EV 8517	EV 8518
Please note:	To screw in the screw patrix you need the placement instrument of the respective series.	

Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw



Version	straight	angled
Article No.	EV 8500	EV 8513
Please note:	The Scanbody is sterilisable and for intra-oral scanning.	

Multi-unit Laboratory implant

- Titanium Grade 5 CF



Version	straight	angled	angled
Type		17°	30°
Article No.	8504	8514-17	8514-30

Multi-unit Laboratory implant CAD/CAM

- Titanium Grade 5 CF



Version	straight	angled	angled
Type		17°	30°
Article No.	8509	8515-17	8515-30

Multi-unit accessories

- EV 8502 Multi-unit cover cap Hex 1,26
- EV 8503 Multi-unit implant pick-up incl. retention screw
- M 11-11 Placement instrument Multi-unit abutment Manual and ratchet
- 8515 T Placement instrument laboratory implant CAD/CAM Multi-unit



Article No.	EV 8502	EV 8503	M 11-11	8515 T
-------------	---------	---------	---------	--------

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 35 Ncm



Implant connection	NP 3,5	NP 3,5	NP 3,5	NP 3,5
Gingiva height	1,5 mm	2,5 mm	3,5 mm	5,5 mm
Article No.	F 8000	F 8003	F 8001	F 8002

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 35 Ncm



Implant connection	RP 4,3/5,0	RP 4,3/5,0	RP 4,3/5,0	RP 4,3/5,0
Gingiva height	1,5 mm	2,5 mm	3,5 mm	5,5 mm
Article No.	F 8010	F 8013	F 8011	F 8012

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 35 Ncm



Implant connection	NP 3,5	NP 3,5	NP 3,5
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	F 8100	F 8101	F 8102
Abutment screw	F 600	F 600	F 600

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 35 Ncm



Implant connection	NP 3,5	NP 3,5	NP 3,5
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	F 8300	F 8301	F 8302
Abutment screw	F 600	F 600	F 600

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 35 Ncm

Type 1



Implant connection	RP 4,3/5,0	RP 4,3/5,0	RP 4,3/5,0
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	F 8110	F 8111	F 8112
Abutment screw	F 601	F 601	F 601

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 35 Ncm

Type 1



Implant connection	RP 4,3/5,0	RP 4,3/5,0	RP 4,3/5,0
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	F 8310	F 8311	F 8312
Abutment screw	F 601	F 601	F 601

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Abutment screw

- Titanium Grade 5 CF



Placement instrument	UG	UG
Article No.	F 600	F 601

Please note: The correct choice of the abutment screw is stated with the respective abutment in the catalogue.

Multi-unit bridge screw

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Placement instrument	Ball Torx	UG
Article No.	6-31-01	F 8501

Multi-unit prosthetic components

- Recommended torque: 15 Ncm
- Titanium base / titanium cap: incl. bridge screw
Material: Titanium Grade 5 CF
- Modelling sleeve without bridge screw
Material: Tecanat (PC)



Article No.	6-31-02	F 8508	F 8505	F 8519	8510
Please note:	The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.				

Multi-unit prosthetic components

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material gold cap, castable: "(AU 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1



Article No.	F 8506	F 8507
-------------	--------	--------

Multi-unit screw patrix

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Article No.	F 8517	F 8518
Please note:	To screw in the screw patrix you need the placement instrument of the respective series.	

Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw



Version	straight	angled
Article No.	F 8500	F 8513
Please note:	The Scanbody is sterilisable and for intra-oral scanning.	

Multi-unit Laboratory implant

- Titanium Grade 5 CF



Version	straight	angled	angled
Type		17°	30°
Article No.	8504	8514-17	8514-30

Multi-unit Laboratory implant CAD/CAM

• Titanium Grade 5 CF

Version			
Type	straight	angled	angled
Article No.	8509	8515-17	8515-30



Multi-unit accessories

- F 8502 Multi-unit cover cap UG
- F 8503 Multi-unit implant pick-up incl. retention screw
- M 11-11 Placement instrument Multi-unit abutment Manual and ratchet
- 8515 T Placement instrument laboratory implant CAD/CAM Multi-unit

Article No.



F 8502



F 8503



M 11-11



8515 T

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 20 Ncm



Implant connection	D 3,4	D 3,4	D 3,4
Gingiva height	1,0 mm	3,0 mm	5,0 mm
Article No.	H 8000	H 8001	H 8002

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 20 Ncm



Implant connection	D 4,1	D 4,1	D 4,1
Gingiva height	1,0 mm	3,0 mm	5,0 mm
Article No.	H 8010	H 8011	H 8012

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 20 Ncm



Implant connection	D 3,4	D 3,4	D 3,4
Gingiva height (mm)	0,6/2,0	1,6/3,0	3,6/5,0
Article No.	H 8100	H 8101	H 8102
Abutment screw	H 62	H 62	H 62

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 20 Ncm



Implant connection	D 3,4	D 3,4	D 3,4
Gingiva height (mm)	0,6/3,0	1,6/4,0	2,4/5,0
Article No.	H 8300	H 8301	H 8302
Abutment screw	H 62	H 62	H 62

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 20 Ncm

Type 1



Implant connection	D 4,1	D 4,1	D 4,1
Gingiva height (mm)	0,6/2,0	1,6/3,0	3,6/5,0
Article No.	H 8110	H 8111	H 8112
Abutment screw	H 62	H 62	H 62

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.



Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 20 Ncm

Type 1



Implant connection	D 4,1	D 4,1	D 4,1
Gingiva height (mm)	0,6/3,0	1,6/4,0	2,4/5,0
Article No.	H 8310	H 8311	H 8312
Abutment screw	H 62	H 62	H 62

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.



Abutment screw

- Titanium Grade 5 CF

Placement instrument	Hex 1,2
Article No.	H 62

Please note: The correct choice of the abutment screw is stated with the respective abutment in the catalogue.



Multi-unit bridge screw






- Titanium Grade 5 CF
- Recommended torque: 15 Ncm

Placement instrument	Ball Torx	Hex 1,2
Article No.	6-31-01	H 8501



Multi-unit prosthetic components

- Recommended torque: 15 Ncm
- Titanium base / titanium cap: incl. bridge screw
Material: Titanium Grade 5 CF
- Modelling sleeve without bridge screw
Material: Tecanat (PC)

					
	titanium base ASC	titanium base	titanium cap	titanium cap Flex	modelling sleeve
Article No.	6-31-02	H 8508	H 8505	H 8519	8510
Please note:	The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.				



Multi-unit prosthetic components

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material gold cap, castable: "(AU 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1

		
	gold cap, castable	CoCr cap
Article No.	H 8506	H 8507



Multi-unit screw patrx

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm

		
	MedentiLOC	Novaloc
Article No.	H 8517	H 8518
Please note:	To screw in the screw patrx you need the placement instrument of the respective series.	




Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw

		
	straight	angled
Article No.	H 8500	H 8513
Please note:	The Scanbody is sterilisable and for intra-oral scanning.	

Multi-unit Laboratory implant

- Titanium Grade 5 CF

			
Version	straight	angled	angled
Type		17°	30°
Article No.	8504	8514-17	8514-30

Multi-unit Laboratory implant CAD/CAM

• Titanium Grade 5 CF

Version			
Type	straight	angled	angled
Article No.	8509	8515-17	8515-30



Multi-unit accessories

- H 8502 Multi-unit cover cap Hex 1,2
- H 8503 Multi-unit implant pick-up incl. retention screw
- M 11-11 Placement instrument Multi-unit abutment Manual and ratchet
- 8515 T Placement instrument laboratory implant CAD/CAM Multi-unit

Article No.



H 8502



H 8503



M 11-11



8515 T

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 35 Ncm



Implant connection	NC 3,3	NC 3,3	NC 3,3
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Article No.	L 8000	L 8001	L 8002

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 35 Ncm



Implant connection	RC 4,1/4,8	RC 4,1/4,8	RC 4,1/4,8
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Article No.	L 8010	L 8011	L 8012

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over corner
- Recommended torque: 35 Ncm



Implant connection	NC 3,3	NC 3,3	NC 3,3
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No. Type 1	L 8100	L 8101	L 8102
Article No. Type 2	L 8200	L 8201	L 8202
Abutment screw	L 65	L 65	L 65

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over corner
- Recommended torque: 35 Ncm



Implant connection	NC 3,3	NC 3,3	NC 3,3
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No. Type 1	L 8300	L 8301	L 8302
Article No. Type 2	L 8400	L 8401	L 8402
Abutment screw	L 65	L 65	L 65

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over corner
- Recommended torque: 35 Ncm



Implant connection	RC 4,1/4,8	RC 4,1/4,8	RC 4,1/4,8
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No. Type 1	L 8110	L 8111	L 8112
Article No. Type 2	L 8210	L 8211	L 8212
Abutment screw	L 65	L 65	L 65

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Type 2 = angled over corner
- Recommended torque: 35 Ncm



Implant connection	RC 4,1/4,8	RC 4,1/4,8	RC 4,1/4,8
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No. Type 1	L 8310	L 8311	L 8312
Article No. Type 2	L 8410	L 8411	L 8412
Abutment screw	L 65	L 65	L 65

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Abutment screw

- Titanium Grade 5 CF



Placement instrument	Torx T6
Article No.	L 65

Please note: The correct choice of the abutment screw is stated with the respective abutment in the catalogue.

Multi-unit bridge screw


- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Placement instrument	Ball Torx	Torx T6
Article No.	6-31-01	L 8501

Multi-unit prosthetic components

- Recommended torque: 15 Ncm
- Titanium base / titanium cap: incl. bridge screw
Material: Titanium Grade 5 CF
- Modelling sleeve without bridge screw
Material: Tecanat (PC)

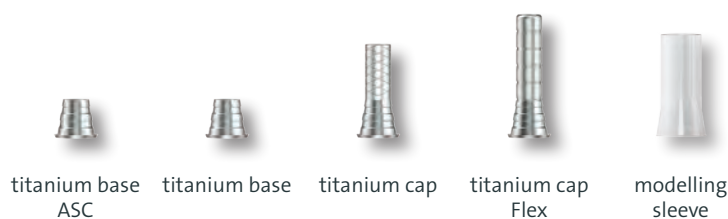

Article No.	6-31-02	L 8508	L 8505	L 8519	8510
Please note:	The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.				

Multi-unit prosthetic components

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material gold cap, castable: "(AU 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1



Article No.	L 8506	L 8507
-------------	--------	--------

Multi-unit screw patrix

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Article No.	L 8517	L 8518
Please note:	To screw in the screw patrix you need the placement instrument of the respective series.	

Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw



Version	straight	angled
Article No.	L 8500	L 8513
Please note:	The Scanbody is sterilisable and for intra-oral scanning.	

Multi-unit Laboratory implant

- Titanium Grade 5 CF



Version	straight	angled	angled
Type		17°	30°
Article No.	8504	8514-17	8514-30

Multi-unit Laboratory implant CAD/CAM

• Titanium Grade 5 CF

Version				
Type		straight	angled 17°	angled 30°
Article No.		8509	8515-17	8515-30

Multi-unit accessories

- L 8502 Multi-unit cover cap Torx T6
- L 8503 Multi-unit implant pick-up incl. retention screw
- M 11-11 Placement instrument Multi-unit abutment Manual and ratchet
- 8515 T Placement instrument laboratory implant CAD/CAM Multi-unit

Article No.

			
L 8502	L 8503	M 11-11	8515 T

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 35 Ncm



Implant connection	RN 4,8
Gingiva height	0,9 mm
Article No.	N 8010

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 35 Ncm



Implant connection	WN 6,5
Gingiva height	1,2 mm
Article No.	N 8020

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit bridge screw

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Placement instrument	Ball Torx	Torx T6
Article No.	6-31-01	N 8501

Multi-unit prosthetic components

- Recommended torque: 15 Ncm
- Titanium base / titanium cap: incl. bridge screw
- Material: Titanium Grade 5 CF
- Modelling sleeve without bridge screw
- Material: Tecanat (PC)



	titanium base ASC	titanium base N 8508	titanium cap N 8505	titanium cap Flex N 8519	modelling sleeve 8510
Article No.	6-31-02	N 8508	N 8505	N 8519	8510

Please note: The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.

Multi-unit prosthetic components

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material gold cap, castable: "(Au 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1



Article No.	N 8506	N 8507
-------------	--------	--------

Multi-unit screw patrix

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



MedentiLOC

Novaloc

Article No.

N 8517

N 8518

Please note:

To screw in the screw patrix you need the placement instrument of the respective series.

Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw



Version

straight

Article No.

N 8500

Please note:

The Scanbody is sterilisable and for intra-oral scanning.

Multi-unit Laboratory implant

- Titanium Grade 5 CF



Version

straight

Type

Article No.

8504

Multi-unit Laboratory implant CAD/CAM

- Titanium Grade 5 CF



Version

straight

Type

Article No.

8509

Multi-unit accessories

- N 8502 Multi-unit cover cap Torx T6
- N 8503 Multi-unit implant pick-up incl. retention screw
- M 11-11 Placement instrument Multi-unit abutment Manual and ratchet



Article No.

N 8502

N 8503

M 11-11

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 30 Ncm



Implant connection	M	M	M
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Article No.	OT 8000	OT 8001	OT 8002

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 30 Ncm



Implant connection	R	R	R
Gingiva height	1,5 mm	3,5 mm	5,5 mm
Article No.	OT 8010	OT 8011	OT 8012

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 20 Ncm



Implant connection	M	M	M
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	OT 8100	OT 8101	OT 8102
Abutment screw	OT 64	OT 64	OT 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 20 Ncm



Implant connection	M	M	M
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	OT 8300	OT 8301	OT 8302
Abutment screw	OT 64	OT 64	OT 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 30 Ncm

Type 1



Implant connection	R	R	R
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	OT 8110	OT 8111	OT 8112
Abutment screw	OT 65	OT 65	OT 65

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.



Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 30 Ncm

Type 1



Implant connection	R	R	R
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	OT 8310	OT 8311	OT 8312
Abutment screw	OT 65	OT 65	OT 65

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.



Abutment screw

- Titanium Grade 5 CF

Placement instrument	Hex 1,2	Hex 1,2
Article No.	OT 64	OT 65

Please note: The correct choice of the abutment screw is stated with the respective abutment in the catalogue.



Multi-unit bridge screw






- Titanium Grade 5 CF
- Recommended torque: 15 Ncm

Placement instrument	Ball Torx	Hex 1,2
Article No.	6-31-01	OT 8501





Multi-unit prosthetic components

- Recommended torque: 15 Ncm
- Titanium base / titanium cap: incl. bridge screw
Material: Titanium Grade 5 CF
- Modelling sleeve without bridge screw
Material: Tecanat (PC)

					
	titanium base ASC	titanium base	titanium cap	titanium cap Flex	modelling sleeve
Article No.	6-31-02	OT 8508	OT 8505	OT 8519	8510
Please note:	The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.				



Multi-unit prosthetic components

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material gold cap, castable: "(AU 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1

		
	gold cap, castable	CoCr cap
Article No.	OT 8506	OT 8507



Multi-unit screw patrix

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm

		
	MedentiLOC	Novaloc
Article No.	OT 8517	OT 8518
Please note:	To screw in the screw patrix you need the placement instrument of the respective series.	




Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw

		
Version	straight	angled
Article No.	OT 8500	OT 8513
Please note:	The Scanbody is sterilisable and for intra-oral scanning.	

Multi-unit Laboratory implant

- Titanium Grade 5 CF

			
Version	straight	angled	angled
Type		17°	30°
Article No.	8504	8514-17	8514-30

Multi-unit Laboratory implant CAD/CAM

- Titanium Grade 5 CF

Version			
Type	straight	angled	angled
Article No.	8509	8515-17	8515-30



Multi-unit accessories

- OT 8502 Multi-unit cover cap Hex 1,2
- OT 8503 Multi-unit implant pick-up incl. retention screw
- M 11-11 Placement instrument Multi-unit abutment Manual and ratchet
- 8515 T Placement instrument laboratory implant CAD/CAM Multi-unit

Article No.



OT 8502



OT 8503



M 11-11



8515 T

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 30 Ncm



Implant connection	D 3,5	D 3,5	D 3,5
Gingiva height	1,0 mm	3,0 mm	5,0 mm
Article No.	R 8000	R 8001	R 8002

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 30 Ncm



Implant connection	D 4,5	D 4,5	D 4,5
Gingiva height	1,0 mm	3,0 mm	5,0 mm
Article No.	R 8010	R 8011	R 8012

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 30 Ncm



Implant connection	D 3,5	D 3,5	D 3,5
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	R 8100	R 8101	R 8102
Abutment screw	R 64	R 64	R 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 30 Ncm



Implant connection	D 3,5	D 3,5	D 3,5
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	R 8300	R 8301	R 8302
Abutment screw	R 64	R 64	R 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 30 Ncm

Type 1



Implant connection	D 4,5	D 4,5	D 4,5
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	R 8110	R 8111	R 8112
Abutment screw	R 64	R 64	R 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 30 Ncm

Type 1



Implant connection	D 4,5	D 4,5	D 4,5
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	R 8310	R 8311	R 8312
Abutment screw	R 64	R 64	R 64

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Abutment screw

- Titanium Grade 5 CF



Placement instrument	Hex 1,26
Article No.	R 64

Please note: The correct choice of the abutment screw is stated with the respective abutment in the catalogue.

Multi-unit bridge screw

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Placement instrument	Ball Torx	Hex 1,26
Article No.	6-31-01	R 8501

Multi-unit prosthetic components

- Recommended torque: 15 Ncm
- Titanium base / titanium cap: incl. bridge screw
Material: Titanium Grade 5 CF
- Modelling sleeve without bridge screw
Material: Tecanat (PC)



titanium base
ASC



titanium base



titanium cap



titanium cap
Flex



modelling
sleeve

Article No.	6-31-02	R 8508	R 8505	R 8519	8510
Please note:	The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.				

Multi-unit prosthetic components

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material gold cap, castable: "(AU 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1



gold cap,
castable



CoCr cap

Article No.	R 8506	R 8507
-------------	--------	--------

Multi-unit screw patrix

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



MedentiLOC



Novaloc

Article No.	R 8517	R 8518
Please note:	To screw in the screw patrix you need the placement instrument of the respective series.	

Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw



straight



angled

Version	straight	angled
Article No.	R 8500	R 8513

Please note:	The Scanbody is sterilisable and for intra-oral scanning.	
--------------	---	--

Multi-unit Laboratory implant

- Titanium Grade 5 CF



straight



angled
17°



angled
30°

Version	straight	angled	angled
Type		17°	30°
Article No.	8504	8514-17	8514-30

Multi-unit Laboratory implant CAD/CAM

• Titanium Grade 5 CF

Version			
Type	straight	angled	angled
Article No.	8509	8515-17	8515-30



Multi-unit accessories

- R 8502 Multi-unit cover cap Hex 1,26
- R 8503 Multi-unit implant pick-up incl. retention screw
- M 11-11 Placement instrument Multi-unit abutment Manual and ratchet
- 8515 T Placement instrument laboratory implant CAD/CAM Multi-unit

Article No.



R 8502



R 8503



M 11-11



8515 T

Multi-unit abutment straight

- Titanium Grade 5 CF
- Sterile packaged
- Recommended torque: 25 Ncm



Implant connection	C/ 3,5-7,0	C/ 3,5-7,0	C/ 3,5-7,0
Gingiva height	1,5 mm	3,0 mm	5,0 mm
Article No.	Y 8000	Y 8001	Y 8002

Please note: To screw in Multi-unit abutments you need the special placement instrument Multi-unit abutment M 11-11.

Multi-unit abutment angled 17°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 15 Ncm

Type 1



Implant connection	/X 3,5-7,0	/X 3,5-7,0	/X 3,5-7,0
Gingiva height (mm)	1,1/2,5	2,1/3,5	4,1/5,5
Article No.	Y 8100X	Y 8101X	Y 8102X

Abutment screw

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit abutment angled 30°

- Titanium Grade 5 CF
- Sterile packaged
- incl. abutment screw
- Type 1 = angled over flat
- Recommended torque: 15 Ncm

Type 1



Implant connection	/X 3,5-7,0	/X 3,5-7,0	/X 3,5-7,0
Gingiva height (mm)	0,6/3,0	1,6/4,0	3,1/5,5
Article No.	Y 8300X	Y 8301X	Y 8302X

Abutment screw

Please note: To screw in the angled Multi-unit abutments you need the placement instrument of the respective series.

Multi-unit bridge screw






- Titanium Grade 5 CF
- Recommended torque: 15 Ncm



Placement instrument	Ball Torx	Hex 1,0
Article No.	6-31-01	Y 8501

Multi-unit prosthetic components

- Recommended torque: 15 Ncm
- Titanium base / titanium cap: incl. bridge screw
Material: Titanium Grade 5 CF
- Modelling sleeve without bridge screw
Material: Tecanat (PC)

					
	titanium base ASC	titanium base	titanium cap	titanium cap Flex	modelling sleeve
Article No.	6-31-02	Y 8508	Y 8505	Y 8519	8510
Please note:	The Multi-unit modelling sleeve can be used with the Multi-unit titanium base and Multi-unit titanium cap.				



Multi-unit prosthetic components

- incl. bridge screw
- Recommended torque: 15 Ncm
- Material gold cap, castable: "(AU 60%; Pd 20%; Pt 19%; Ir 1%)"
- Material CoCr cap: CrCo alloy / CTE 14.1

		
	gold cap, castable	CoCr cap
Article No.	Y 8506	Y 8507



Multi-unit screw patrix

- Titanium Grade 5 CF
- Recommended torque: 15 Ncm

		
	MedentiLOC	Novaloc
Article No.	Y 8517	Y 8518
Please note:	To screw in the screw patrix you need the placement instrument of the respective series.	




Multi-unit scanbody

- Titanium specially coated
- incl. bridge screw

		
	straight	angled
Article No.	Y 8500	Y 8513
Please note:	The Scanbody is sterilisable and for intra-oral scanning.	

Multi-unit Laboratory implant

- Titanium Grade 5 CF

			
	straight	angled 17°	angled 30°
Article No.	8504	8514-17	8514-30

Multi-unit Laboratory implant CAD/CAM

- Titanium Grade 5 CF

Version

Type

Article No.



straight



angled

17°



angled

30°

8509

8515-17

8515-30

Multi-unit accessories

- Y 8502 Multi-unit cover cap Hex 1,0
- Y 8503 Multi-unit implant pick-up incl. retention screw
- M 11-11 Placement instrument Multi-unit abutment Manual and ratchet
- 8515 T Placement instrument laboratory implant CAD/CAM Multi-unit

Article No.



Y 8502



Y 8503



M 11-11



8515 T

Placement instrument Hex 1,26

• Hardened stainless steel



Version	Contra-angle	Contra-angle	Manual and ratchet	Manual and ratchet
Type	long	short	long	short
Article No.	M 03-1	M 09-1	M 10-1	M 11-1
Suitable for:	BS-Series, C-Series, D-Series, EV-Series, I-Series, R-Series, S-Series, MedentiLOC abutment straight			

Placement instrument Hex 1,2

• Hardened stainless steel



Version	Contra-angle	Contra-angle	Manual and ratchet	Manual and ratchet
Type	long	short	long	short
Article No.	M 03-2	M 09-2	M 10-2	M 11-2
Suitable for:	T-Series, H-Series, OT-Series			

Placement instrument Hex 1,0

• Hardened stainless steel



Version	Contra-angle	Contra-angle	Manual and ratchet	Manual and ratchet
Type	long	short	long	short
Article No.	M 03-3	M 09-3	M 10-3	M 11-3
Suitable for:	Y-Series			

Placement instrument Torx T6

• Hardened stainless steel



Version	Contra-angle	Contra-angle	Manual and ratchet	Manual and ratchet
Type	long	short	long	short
Article No.	M 03-4	M 09-4	M 10-4	M 11-4
Suitable for:	B-Series, L-Series, N-Series			

Placement instrument Ball Torx

- Hardened stainless steel



Version	Contra-angle	Contra-angle	Manual and ratchet
Type	long	short	long
Article No.	6-13-06	M 03-8	M 10-8
Suitable for: Novaloc abutment angled, titanium base ASC Flex			

Placement instrument UG

- Hardened stainless steel



Version	Contra-angle	Contra-angle	Manual and ratchet	Manual and ratchet
Type	long	short	long	short
Article No.	M 03-5	M 09-5	M 10-5	M 11-5
Suitable for: E-Series, F-Series, K-Series				

Placement instrument Multi-unit abutment straight

- Stainless steel



Version	Manual and ratchet
Article No.	M 11-11

Torque ratchet

- with infinitely variable torque setting
- 10-40 Ncm
- Hardened stainless steel



Article No.	M 12
-------------	------





Publisher

Medentika® GmbH

As at: August 2020

We are certified:

DIN EN ISO 13485

**Medical Devices Directive 93/42/EEC,
Annex II**

CE 0483

We have a passion for precision, quality and durability

- One of the leading compatibles manufacturer
- Made in Germany
- Compatible with all major implant systems at an affordable price
- Committed to collaboration, teamwork and partnership
- Guaranteed up to lifetime

» Passion for
Precision «



Medentika® GmbH
Hammweg 8–10
76549 Hügelsheim
info@medentika.de
www.medentika.com

© Medentika® GmbH, 2020. All rights reserved.
Medentika® and/or other trademarks and logos from Medentika® mentioned herein are the trademarks or registered trademarks of Medentika® and/or its affiliates.

 **MEDENTIKA®**
A Straumann Group Brand